

State of North Dakota)
)ss
County of Burleigh)

I, Deb Kashur, do hereby certify that I am the duly-appointed Forensic Scientist for the State of North Dakota and an official custodian of the records and files of the office thereof, that I have carefully compared the

Ethanol Breath Standard Analytical Report, Lot No. 29614080A2, Expiration 12/05/2016
(12/19/14)

hereto attached with the respective original as the same appears of record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, and find the same to be a true and correct copy thereof and of the whole thereof. In witness whereof I have set my hand at the city of Bismarck, in said county this:

19 day of December, 2014

Deb Kashur
Deb Kashur, Forensic Scientist


State of North Dakota)
)ss
County of Burleigh)

On this 19 day of December, 2014, before me personally appeared Deb Kashur, known to me to be a Forensic Scientist for the State of North Dakota, and acknowledged to me that she has executed the same.

Subscribed to and sworn before me this:

19 day of December, 2014

Cindy Leingang
Cindy Leingang, Notary Public, State of North Dakota
My Commission Expires January 11, 2017

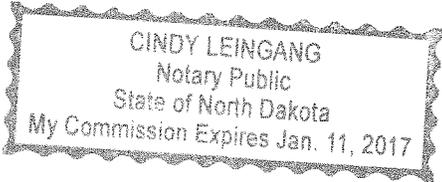

(SEAL)

ETHANOL BREATH STANDARD ANALYTICAL REPORT

Ethanol Breath Standard Lot Number 29614080A2 Expiration Date 12/05/2016

This standard was analyzed by ILMO Specialty Gases with a reported result of 208 ppm which is the equivalent of 0.08 AC of Ethanol in Nitrogen. ILMO Specialty Gases has provided a Certificate of Analysis traceable to N.I.S.T. SRM Ethanol Standards.

A proper result for the standard test using a cylinder of this lot number would be the range of 0.075 to 0.085 g ethanol/210 L of vapor (g/100 ml of blood or g/210 L of end expiratory breath).

The Intoxilyzer® will print out the value of the standard test in 3 digits on Intoxilyzer® Test Record (Form 106-18000).


The number of cylinders sent to each location will be based on need. The standard may be used until the date of expiration as indicated by the manufacturer's Certificate of Analysis.

Deb Kashur

Deb Kashur, Forensic Scientistt

19 December 2014

Date Approved

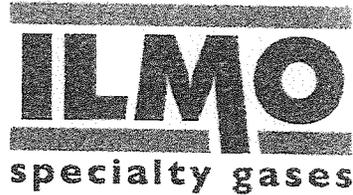

7 Eastgate Dr. • P.O. Box 790 • Jacksonville, IL 62651-0790
217-245-2183 • Fax: 217-243-7634 • www.ilmoproducts.com

Certificate of Analysis

Certificate ID: 7342
Part #: BAC105L080T
Cylinder Size: 105L
Lot Number: 29614080A2
Expiration: 12/5/2016

0.080 BAC (For the calibration of instruments used to determine breath alcohol concentration)

Contents: 105 Liters @ 1000 psig 70°F (21°C)

| Component: | Concentration: | Accuracy: | Method: |
|------------|----------------|--------------------------|---------|
| Ethanol | 208 ppm | +/- 0.002 or 2% | NDIR |
| Nitrogen | Balance | BAC whichever is greater | |

*NIST Standard Reference Material
Cylinder No. CCI4290 / Job No. 09160202
Certified 212.8 µmol/mol Ethanol in Nitrogen
for ILMO Products Co., Jacksonville, IL

Store in dry area, away from sources of heat, ignition
and direct sunlight. Do not allow storage area to
exceed 52 °C (125 °F).


Specialty Gas Lab Tech

11/20/14
Date

Distributed by: CMI Inc.
316 East Ninth Street
Owensboro, KY 42303
Phone 866-835-0690
www.alcoholtest.com

