

State of North Dakota     )  
  )ss  
County of Burleigh        )

I, Charles E. Eder, do hereby certify that I am the duly-appointed State Toxicologist for the State of North Dakota and an official custodian of the records and files of the office thereof, that I have carefully compared the

**Intoximeters Alco-Sensor FST® Ethanol Breath Standard Analytical Report, Lot No. AG131903, Expiration 11/15/2013 (11/01/12)**

hereto attached with the respective original as the same appears of record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, and find the same to be a true and correct copy thereof and of the whole thereof. In witness whereof I have set my hand at the city of Bismarck, in said county this:

1<sup>st</sup> day of NOVEMBER, 2012


  
\_\_\_\_\_  
Charles E. Eder, State Toxicologist


State of North Dakota     )  
  )ss  
County of Burleigh        )

On this 1<sup>st</sup> day of November, 2012, before me personally appeared Charles E. Eder, known to me to be the State Toxicologist for the State of North Dakota, and acknowledged to me that he/she has executed the same.

Subscribed to and sworn before me this:

1<sup>st</sup> day of November, 2012

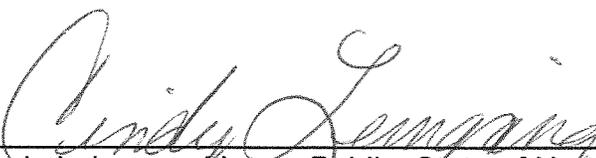  
\_\_\_\_\_  
Cindy Leingang, Notary Public, State of North Dakota  
My Commission Expires January 11, 2017

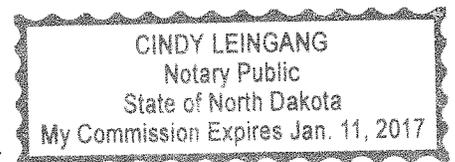

(SEAL)

**INTOXIMETERS ALCO-SENSOR FST®  
ETHANOL BREATH STANDARD ANALYTICAL REPORT**

Ethanol Breath Standard Lot Number AG131903 Expiration Date 11/15/2013

This standard was analyzed by AIRGAS Mid America with a reported result of 223 ppm which is the equivalent of 0.082 BrAC of Ethanol in Nitrogen. AIRGAS Mid America has provided a Certificate of Analysis traceable to N.I.S.T. RGM Ethanol Standards.

The number of cylinders sent to each location will be based on need. The standard may be used until the date of expiration as indicated by the manufacturer's Certificate of Analysis.



Charles E. Eder, State Toxicologist

01 Nov 12

Date Approved



Airgas Mid America (LABORATORY)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

## Certificate of Analysis

**Customer Name**

Intoximeters, Inc.  
2081 Craig Road  
St. Louis, Mo 63146

**Test Date:** 15-Nov-2011

Dear Sir,

This is your Certificate of Analysis:

<u>Exp. Date</u>	<u>Cyl. Type</u>	<u>Component</u>	<u>Certified Concentration</u>
11/15/2013	108	Ethanol Nitrogen	0.082 ± 0.002 BrAC (223 ppm) Balance

**Lot #** AG131903

Certification Traceable to N.I.S.T. RGM Ethanol Standards:

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	391.5 ppm	EB0010603	390.9 ppm
EB0010570	258.4 ppm	EB0010559	258.3 ppm
EB0010285	208.9 ppm	EB0010595	209.2 ppm
EB0010561	101.9 ppm	EB0010562	104.9 ppm
EB0010681	53.0 ppm	EB0010579	52.4 ppm

**Analytical Method:** NDIR

Analyst: *Paul M...*

ISO 17025:2005 A2LA accredited. Certificate Number 2989.01